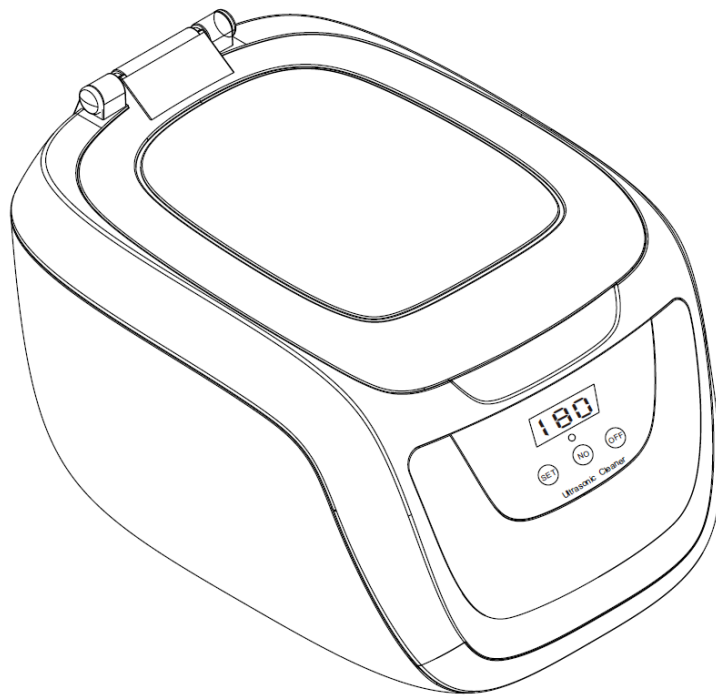




# ***Ultrasonic Cleaner Baths***

**CE-5700A**

**Manual**



## Index

Pag 2 Introduction

Pag 2 Warning

Pag 3 Description

Pag 4 Operating instructions





Pag 4 Specification

Pag 5 Cleaning process

Pag 6 Disposal of electronic devices

Pag 6 Smaltimento dei dispositivi elettronici

## PACK CONTENTS








			
Ultrasonic bath	Accessories	65ml universal cleaning solution	Instruction manual

## INTRODUCTION

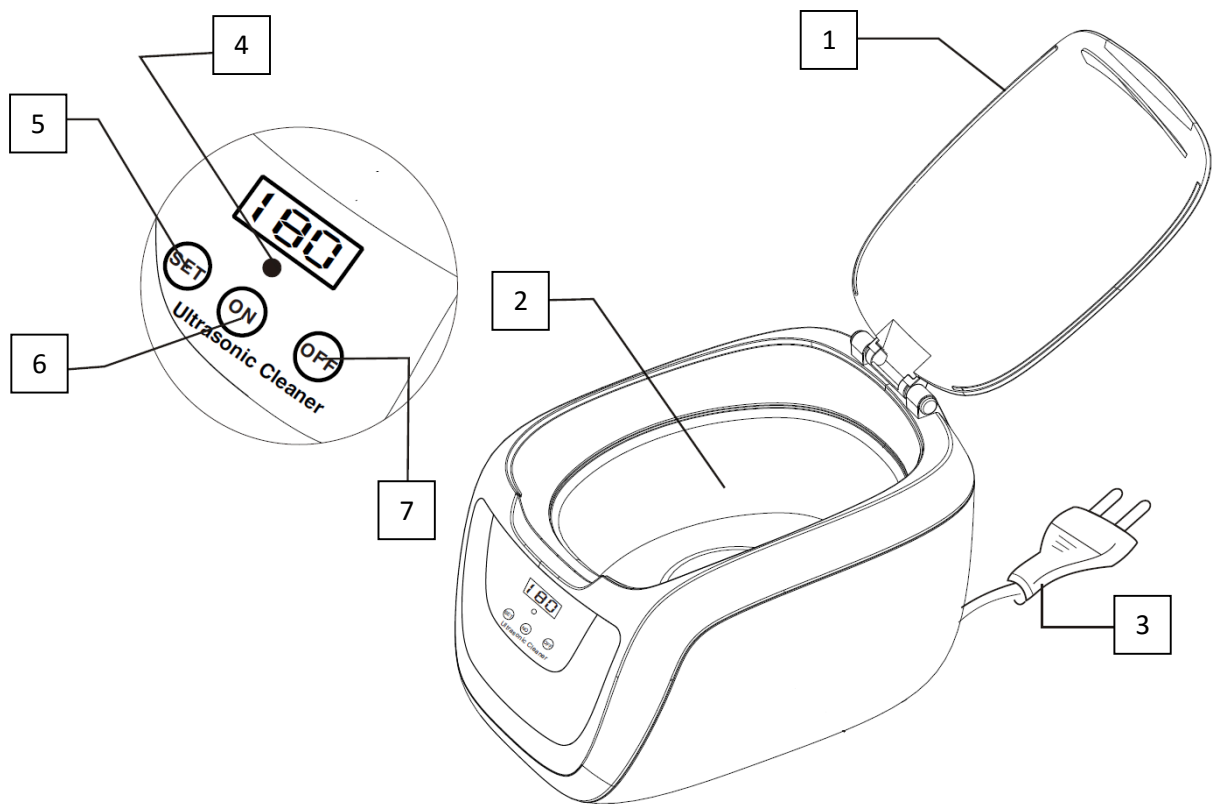
Ultrasonic cleaner is based on the cavitation effect caused by high frequency ultrasonic wave vibration signal in fluid. Microscopic bubbles are formed and they implode violently that cause cavitation, which gives out great impact on the cleaning subject and provides an intense scrubbing action on the surface of the cleaning subject. Additionally, the bubbles are small enough to penetrate even microscopic crevices, cleaning them thoroughly and consistently.

## SAFETY WARNINGS

Observe and follow the operation manual








	This instrument has been designed for the ultrasonic treatment of <u>items</u> in <u>liquids</u> only. <b>Don't operate without liquids.</b> This product must be operated by qualified staff only.
	Connect the unit to a grounded shockproof socket only! Do not open the unit! Maintenance must be done by authorized personnel only! Use this product in a stable and dry work place! Use only distilled water! Pull the mains plug in case of any malfunctions!
	Do not operate the unit with flammable cleaning media!
	Do not put any acids or chlorides into the stainless-steel tank! Do not place any items directly on the tank floor, but use the basket!
	Do not reach inside the cleaning liquid or touch sound carrying parts (tank, basket, cleaning items, etc.) during operation.
	Ultrasonic cleaner unit can produce annoying sound.
	Exclusion of liability; the manufacturer cannot be held liable for damages on persons, equipment or cleaning items caused by improper use and non-observance of the Operating Instructions. The operator is responsible for the instructions of the operating staff. For any queries please contact your supplier or the manufacturer

## DESCRIPTION



- 1) Lid
- 2) Stainless steel tank
- 3) Plug and cord
- 4) Indication light
- 5) Timer setting key
- 6) Power on key
- 7) Power off key

## OPERATING INSTRUCTIONS

	<p>Open the lid, and fill the stainless steel tank with water</p>
	<p>The item should be immersed well into the water. However, do not exceed the "MAX-" mark.</p>
	<p>Close the lid, and plug in.</p>
	<p>Touch "SET" key and select from 5 optional working cycles freely: 180s -&gt; 280s -&gt; 380s -&gt; 480s -&gt; 90s</p>
	<p>Touch "ON" key to start cleaning, and the indication light is on. The timer will be displayed on the screen.</p>
	<p>When reach the time of "000", the unit will auto stop, the light will turn off. If another cleaning is needed, just repeat the above steps. During cleaning, if you want to stop, just touch " OFF " key. Touch "ON" key again, the unit will implement the remainder program to continue the cleaning. Furthermore, you can touch "SET" key to return working cycles</p>
	<p>When cleaning process is finished, unplug it.</p>

Capacity	Timer (sec)	Ultrasonic frequency (kHz)	Ultrasonic power	N° trasducers	Tank size (L x W x H) mm	External size (L x W x H) mm	Weight
0,75	90- 180- 280- 380- 480	42	50W	1	150x130x50	210x180x125	0,97

## CLEANING PROCESS

Please observe any national safety regulations that may apply in addition to the present instructions.

Observe the general safety warnings.

The operator is responsible for the control of the cleaning result.

Take the warming of the cleaning liquid into consideration when cleaning temperature-sensitive items.

Ultrasound can damage sensitive surfaces when operated **over a prolonged** period of time and particularly when operated at low cleaning frequencies.

If required for the cleaning operation by hand, pre-heat the liquid (in units of heating).

Immerse the cleaning items into the cleaning liquid. Do not place any items or containers directly onto the tank floor. Use either a cleaning basket, a becker (filled with water + cleaning chemical) or hang the items into the liquid.

Set the cleaning time – switch on the ultrasound.


Monitor the cleaning process: Check the cleaning result by visual inspection. Repeat the cleaning process if necessary.

Rinse the cleaned items after the cleaning and dry if necessary.

## MAINTANANCE / CARE

<p><b>Caution!</b> Pull the mains plug before you carry out any maintenance and care works! Do not put the unit under water! For repair return the unit to your supplier or to the manufacturer.</p>
<p><b>Electrical safety:</b> Regularly check the housing and the mains cable for damage to avoid electrical accidents.</p>
<p><b>Care of transducer tank:</b> The deposits in the stainless-steel tank can be removed gently, e.g. by mild decalcifiers. Do not use any scouring media!</p>
<p><b>Care of housing:</b> Depending on their kind contaminations can be removed with a mild household cleaner or decalcifier (wipe with wet cloth).</p>
<p><b>Disinfection:</b> If the unit is operated in the medical and sanitary sector it is necessary to disinfect the transducer tank and the surfaces regularly for hygienic purposes (standard surface disinfectants).</p>

## DISPOSAL OF ELECTRONIC DEVICES

	<p>The electrical and electronic equipment marked with this symbol cannot be disposed of in public landfills.</p> <p>According to the UE Directive 2002/96/EC, the European users of electrical and electronic equipment can return it to the dealer or manufacturer upon purchase of a new one.</p> <p>The illegal disposal of electrical and electronic equipment is punished with an administrative fine.</p>
---	--